

Method 508 MOD

Date Extracted 25 Feb 02

Page

#66CMS-17655

Lab #	Description	Sample vol/wt	Drip rate ml/min	Surr add	Spk add	IS add	Final vol.	T.V. pos.	pH	Count		
	LB	500mL		1mL			1mL					
	Ref 1				1mL							
	Ref 2				1mL							
	4038											
	4039											
	4125											
	4126											
	4127											
	4128											
	4129											
	4130											
	4131											
	4132											
Remarks												
Reviewed by <i>[Signature]</i> 3/12/02												
drip rate must be between 5-15 ml/min for liq-liq extractors drip rate - Extraction type - <u>Seal funnel</u> Solv. lot# <u>139466</u> NaCl lot# <u>139618</u> Na2SO4 lot# <u>46623</u>												
STANDARD	INT STD LOG#											
CALIBRATION	<u>1/10/20/02</u>											
REF/SPIKE	<u>2193</u>											
MDL/MDRF												
Q. CHECK												
INT. STD.	<u>032102</u>											
SURROGATE	<u>21002</u>											
LPC												
ENDRIN/DDT												

Analyst ML
Revision 4/12/01

Verified by [Signature]

Reviewed by [Signature]
Date 4/11/02

Sequence Name: C:\HPCHEM\1\SEQUENCE\MAR2202.S

Comment:

Operator:

Data Path: C:\HPCHEM\1\DATA\mar2202\

Pre-Seq Cmd:

Post-Seq Cmd:

Method Sections To Run

On A Barcode Mismatch

(X) Full Method

(X) Inject Anyway

() Reprocessing Only

() Don't Inject

Line	Type	Vial	DataFile	Method	Sample Name
------	------	------	----------	--------	-------------

1	Sample	1	DFTPP	GCMS0308	
2	Sample	2	CAL40	GCMS0308	
3	Sample	29	5900	GCMS0308	gc/ms scan 3/13
4	Sample	30	5901	GCMS0308	gc/ms scan 3/13
5	Sample	3	LB	GCMS0308	gc/ms scan 2/20
6	Sample	4	REF1	GCMS0308	gc/ms scan 2/20
7	Sample	5	REF2	GCMS0308	gc/ms scan 2/20
8	Sample	6	3825	GCMS0308	gc/ms scan 2/20
9	Sample	7	3826	GCMS0308	gc/ms scan 2/20
10	Sample	8	3827	GCMS0308	gc/ms scan 2/20
11	Sample	9	3828	GCMS0308	gc/ms scan 2/20
12	Sample	10	3829	GCMS0308	gc/ms scan 2/20 fb
13	Sample	11	3830	GCMS0308	gc/ms scan 2/20
14	Sample	12	3831	GCMS0308	gc/ms scan 2/20
15	Sample	13	3832	GCMS0308	gc/ms scan 2/20 fb
16	Sample	14	3823	GCMS0308	gc/ms scan 2/20
17	Sample	15	3824	GCMS0308	gc/ms scan 2/20
18	Sample	1	DFTPP2	GCMS0308	
19	Sample	2	CAL40A	GCMS0308	
20	Sample	16	LBA	GCMS0308	gc/ms scan 2/25
21	Sample	17	REFA1	GCMS0308	gc/ms scan 2/25
22	Sample	18	REFA2	GCMS0308	gc/ms scan 2/25
23	Sample	19	4038	GCMS0308	gc/ms scan 2/25
24	Sample	20	4039	GCMS0308	gc/ms scan 2/25
25	Sample	21	4125	GCMS0308	gc/ms scan 2/25
26	Sample	22	4126	GCMS0308	gc/ms scan 2/25
27	Sample	23	4127	GCMS0308	gc/ms scan 2/25
28	Sample	24	4128	GCMS0308	gc/ms scan 2/25
29	Sample	25	4129	GCMS0308	gc/ms scan 2/25
30	Sample	26	4130	GCMS0308	gc/ms scan 2/25
31	Sample	27	4131	GCMS0308	gc/ms scan 2/25
32	Sample	28	4132	GCMS0308	gc/ms scan 2/25
33	Sample	31	LBB	GCMS0308	gc/ms scan 2/25
34	Sample	32	REFB	GCMS0308	gc/ms scan 2/25
35	Sample	33	REFB1	GCMS0308	gc/ms scan 2/25
36	Sample	34	4028	GCMS0308	gc/ms scan 2/25
37	Sample	35	4029	GCMS0308	gc/ms scan 2/25
38	Sample	36	4030	GCMS0308	gc/ms scan 2/25
39	Sample	37	4031	GCMS0308	gc/ms scan 2/25 fb
40	Sample	38	4032	GCMS0308	gc/ms scan 2/25
41	Sample	39	4033	GCMS0308	gc/ms scan 2/25
42	Sample	40	4034	GCMS0308	gc/ms scan 2/25

Last Modified: Wed Mar 27 12:53:53 2002

Page: 1

DFTPP

Data File : C:\HPCHEM\1\DATA\MAR2202\DFTPP2.D

Acq On : 23 Mar 2002 8:51 am

Sample :

Misc :

MS Integration Params: GOOFY.P

Method : C:\HPCHEM\1\METHODS\GCMS0308.M (RTE Integrator)


Title : 209 625/TCLP calibration table

Vial: 1

Operator:

Inst : GC/MS 209

Multiplr: 1.00

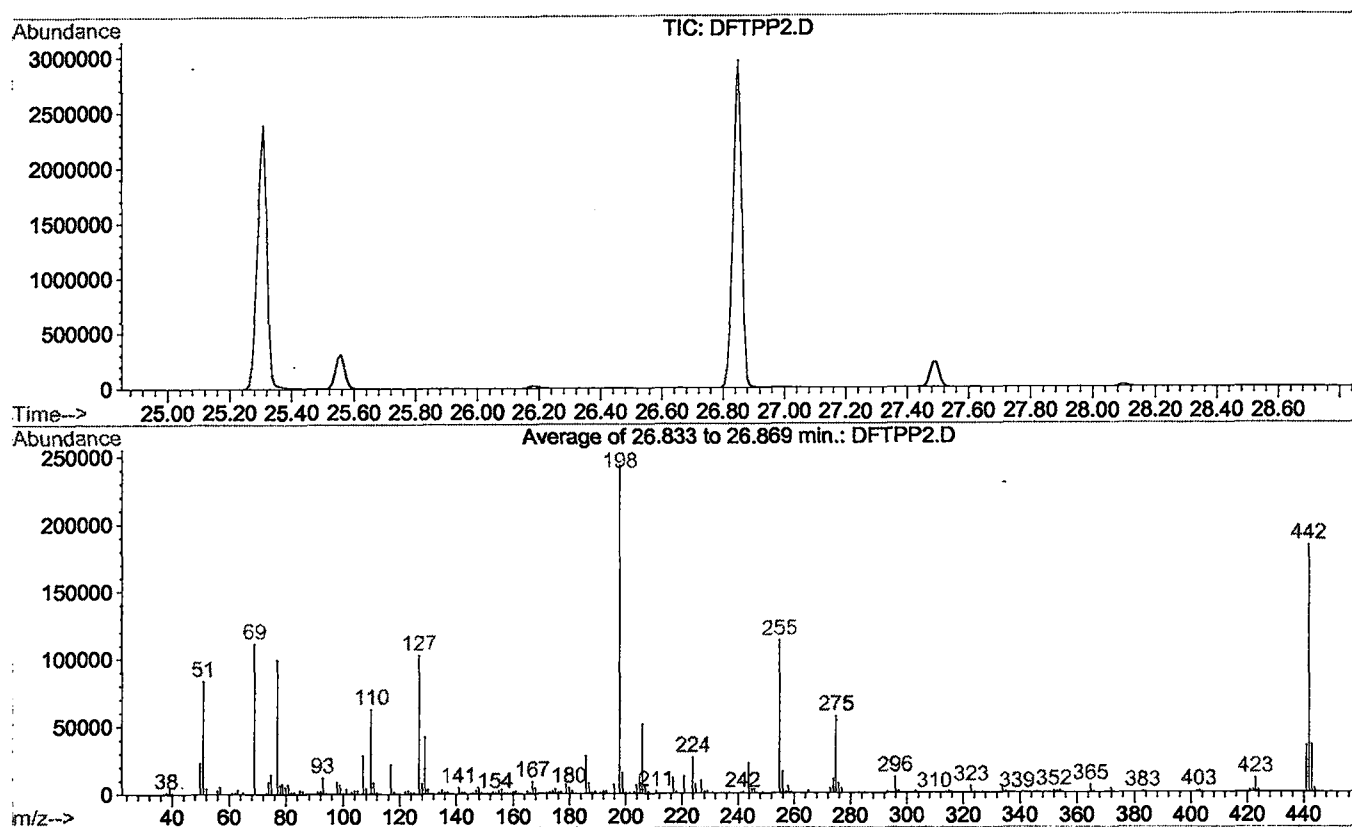

Spectrum Information: Average of 26.833 to 26.869 min.

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	30	60	34.5	83904	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	46.0	111776	PASS
70	69	0.00	2	0.0	30	PASS
127	198	40	60	42.4	103040	PASS
197	198	0.00	1	0.0	0	PASS
198	198	100	100	100.0	243141	PASS
199	198	5	9	6.6	16008	PASS
275	198	10	30	23.4	56987	PASS
365	198	1	100	2.5	6010	PASS
441	443	0.01	100	97.9	34706	PASS
442	198	40	110	75.4	183304	PASS
443	442	17	23	19.3	35446	PASS