

Reviewed by UV
Date 6/16/2

DFTPP

Data File : C:\MSDCHEM\1\DATA\060602\DFTPP.D

Acq On : 6 Jun 2002 9:27 am

Sample :

Misc :

MS Integration Params: EVENTS.E

Vial: 1

Operator: McLean

Inst : Instrumen

Multiplr: 1.00

Method : C:\MSDCHEM\1\METHODS\060302.M (Chemstation Integrator)

Title : 508 Modified GC/MS scan

Spectrum Information: Scan 3597

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	30	60	44.9	149312	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	37.5	124744	PASS
70	69	0.00	2	0.6	766	PASS
127	198	40	60	49.0	163008	PASS
197	198	0.00	1	0.0	0	PASS
198	198	100	100	100.0	332864	PASS
199	198	5	9	6.5	21528	PASS
275	198	10	30	21.6	71912	PASS
365	198	1	99	2.8	9386	PASS
441	443	1	100	79.3	39904	PASS
442	198	40	110	78.3	260608	PASS
443	442	17	23	19.3	50352	PASS

DFTPP.D 060302.M

Mon Jun 10 10:17:37 2002

DFTPP

Data File : C:\MSDCHEM\1\DATA\060702\DFTPP.D

Acq On : 7 Jun 2002 8:36 am

Sample :

Misc :

MS Integration Params: EVENTS.E

Method : C:\MSDCHEM\1\METHODS\060302.M (Chemstation Integrator)


Title : 508 Modified GC/MS scan

Vial: 1

Operator:

Inst : Instrume

Multiplr: 1.00

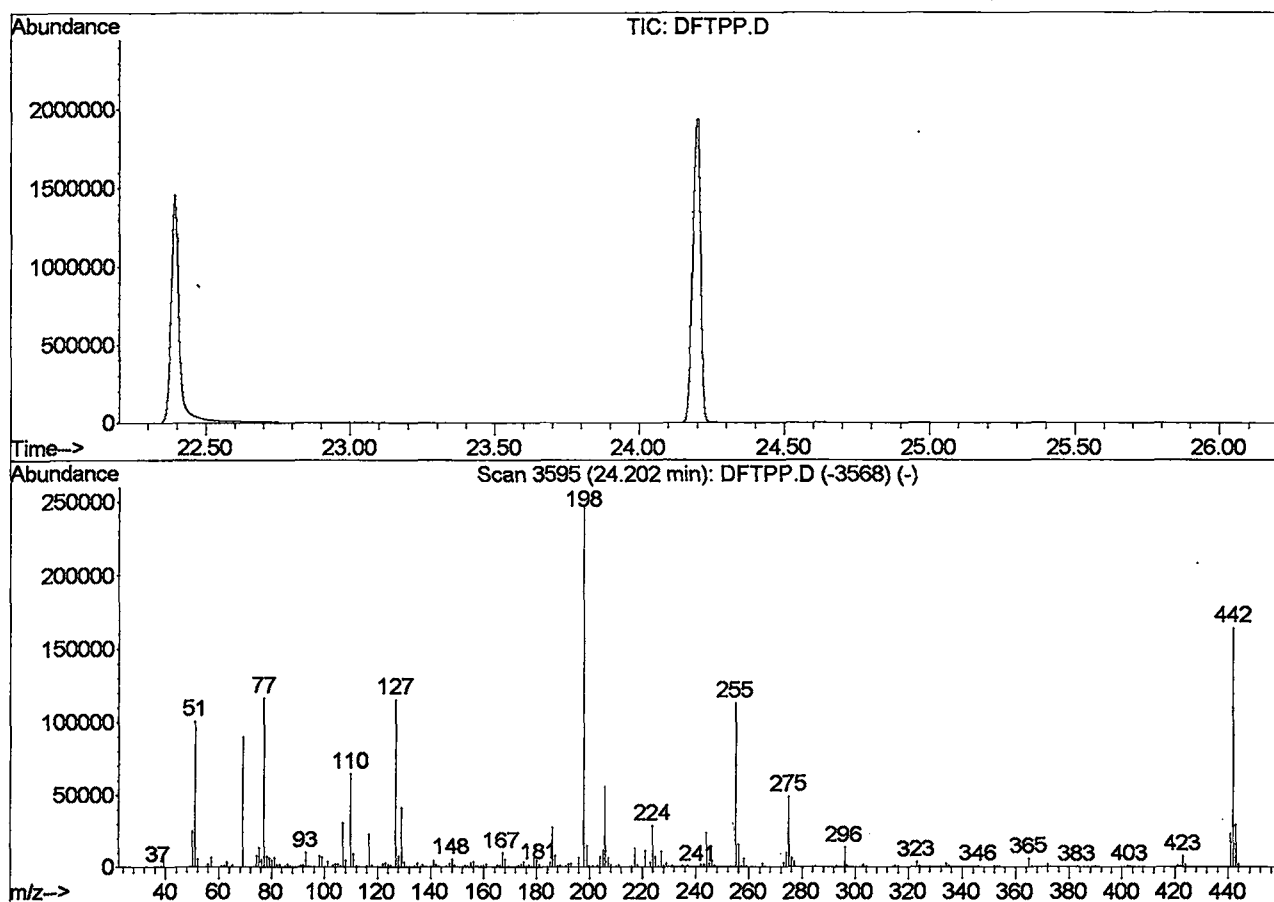

Spectrum Information: Scan 3595

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	30	60	40.6	100776	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	36.4	90368	PASS
70	69	0.00	2	0.5	446	PASS
127	198	40	60	46.6	115600	PASS
197	198	0.00	1	0.0	0	PASS
198	198	100	100	100.0	248192	PASS
199	198	5	9	6.1	15230	PASS
275	198	10	30	19.9	49344	PASS
365	198	1	99	2.5	6143	PASS
441	443	1	100	79.2	23888	PASS
442	198	40	110	66.2	164416	PASS
443	442	17	23	18.3	30144	PASS

DFTPP.D 060302.M

Mon Jun 10 10:53:59 2002