

Sequence Name: C:\MSDCHEM\1\SEQUENCE\020516.S

Comment: GCMS scan

Operator: Nefliu

Data Path: C:\MSDchem\1\DATA\020516\

Pre-Seq Cmd:

Post-Seq Cmd:

Method Sections To Run	On A Barcode Mismatch
(X) Full Method	(X) Inject Anyway
() Reprocessing Only	() Don't Inject

Line	Type	Vial	DataFile	Method	Sample Name
1	Sample	1	DFTPP	508FAST	
2	Sample	2	0516C1	508SCAN1	ccv
3	Sample	3	0516C2	508SCAN1	ccv
4	Sample	4	0513LB	508SCAN1	05/13 lab blk
5	Sample	5	0514LB	508SCAN1	05/14 lab blk
6	Sample	6	0513REF1	508SCAN1	05/13 ref
7	Sample	7	0513REF2	508SCAN1	05/13 ref
8	Sample	8	0514REF1	508SCAN1	05/14 ref
9	Sample	9	0514REF2	508SCAN1	05/14 ref
10	Sample	10	11282	508SCAN1	sample
11	Sample	11	11283	508SCAN1	sample
12	Sample	12	11284	508SCAN1	sample
13	Sample	13	11285	508SCAN1	sample
14	Sample	14	11303	508SCAN1	sample
15	Sample	15	11304	508SCAN1	sample
16	Sample	16	11305	508SCAN1	sample
17	Sample	17	10241	508SCAN1	sample
18	Sample	18	10242	508SCAN1	sample
19	Sample	19	10243	508SCAN1	sample
20	Sample	20	10244	508SCAN1	sample
21	Sample	21	10245	508SCAN1	sample
22	Sample	22	10246	508SCAN1	sample
23	Sample	23	10247	508SCAN1	sample
24	Sample	24	10301	508SCAN1	sample
25	Sample	25	10302	508SCAN1	sample

Method JDEGCMSCM
Instrument 214

File Directory 02 0576

Storage Directory _____

Lab #	Filename	Description	Vial #		Inj. ul	Standards used - Lot #			Int. Std.	Remarks	Initials
			front	rear		Calibration	Reference	Surrogate			
	27TPP	d ftop	1								MN
	057601	cel	2			22876/22877/22860					
	057602		3								
	057603	cel blk	4					22875	22867		
	057403		5								
	057301	ref	6			22972					
	↓ 2	↓	7								
	057401	↓	8								
	↓ 2	↓	9								
	1282	sample	10								
	↓ 3	↓	11								
	↓ 4	↓	12								
	↓ 5	↓	13								
	11303	↓	14								
	↓ 4	↓	15								
	↓ 5	↓	16								
	10241	↓	17								
	↓ 2	↓	18								
	↓ 3	↓	19								
	↓ 4	↓	20								
	↓ 5	↓	21								
	↓ 6	↓	22								
	↓ 7	↓	23								
	10301	↓	24								
	10302	↓	25								

Date 05/16/02


Extraction date 05/13, 14/02

Page 10

DFTPP

Data File : C:\MSDCHEM\1\DATA\020516\DFTPP.D
 Acq On : 16 May 2002 9:44 am
 Sample :
 Misc :
 MS Integration Params: rteint.e
 Method : C:\MSDCHEM\1\METHODS\SCAN020507.M (RTE Integrator)
 Title : Method 508 GC/MS Scan

Vial: 1
 Operator: Nefliu
 Inst : Instrume
 Multiplr: 1.00

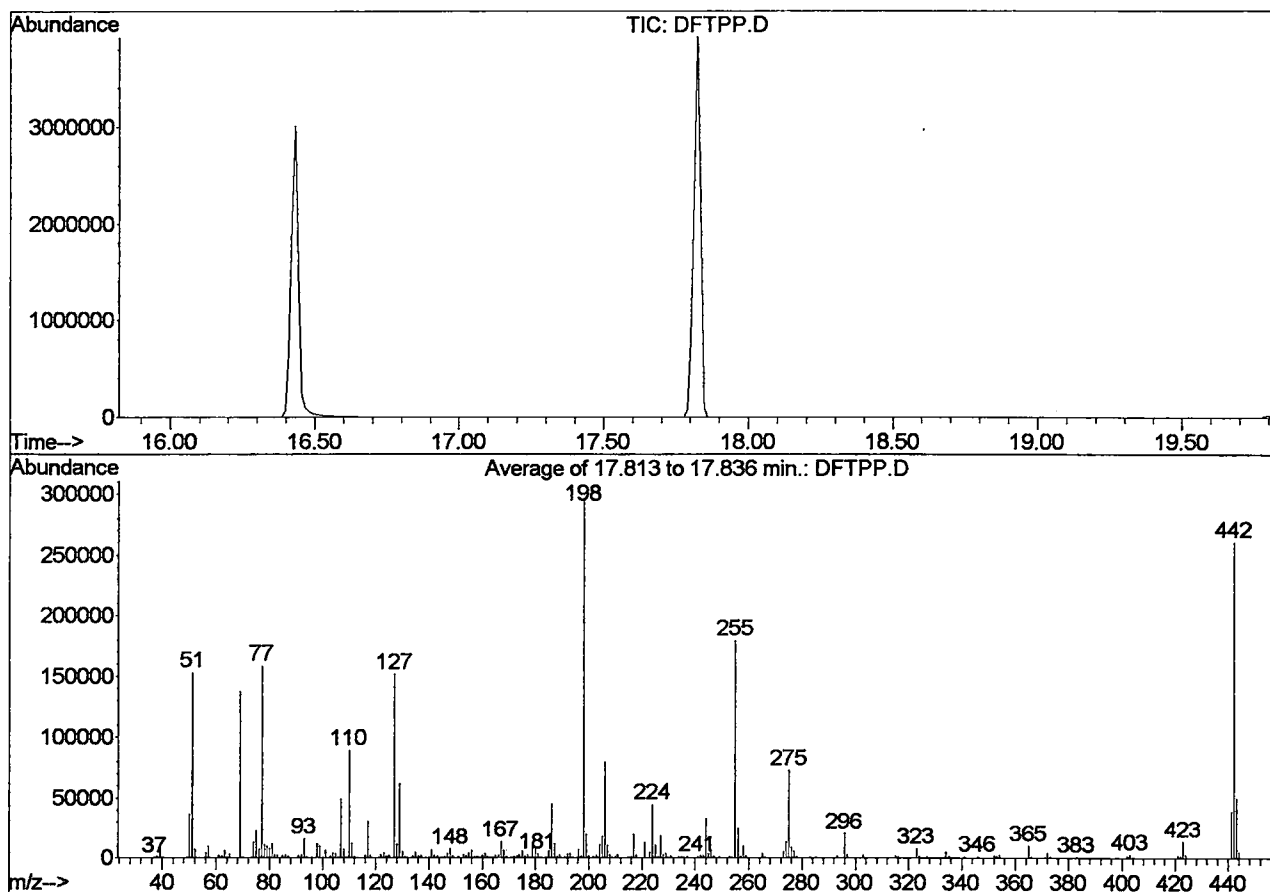

Spectrum Information: Average of 17.813 to 17.836 min.

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	30	60	51.7	153088	PASS
68	69	0.00	2	0.2	296	PASS
69	198	0.00	100	46.4	137362	PASS
70	69	0.00	2	0.4	614	PASS
127	198	40	60	51.2	151762	PASS
197	198	0.00	1	0.5	1441	PASS
198	198	100	100	100.0	296213	PASS
199	198	5	9	6.7	19978	PASS
275	198	10	30	24.7	73056	PASS
365	198	1	99	3.4	9977	PASS
441	443	1	100	78.4	39042	PASS
442	198	40	110	88.1	261056	PASS
443	442	17	23	19.1	49797	PASS

DFTPP.D SCAN020507.M

Fri May 17 13:13:19 2002