

User: Vinci, David L
Westchester Dept. of Labs & Research
Date: 04/16/2002 Time: 15:06:04

Sample: AE06992
Analysis: \$GCMS GCMS Scan For Unknowns
Units: ug
Started: 4/16/02 15:05 Ended: 4/16/02 15:05 Analyst: DLV
Page: 1

	Component Name	Viol	Result	Qualifier	MDL
1	Other unknown compounds		.		
2	Surr_2,4-DDD		118		5.0

Comments for Sample AE06992 - Analysis \$GCMS

Westchester Dept. of Labs & Research

User: Vinci, David L

Date: 04-16-2002 Time: 15:06:20

The GCMS scan, from 35 to 550 amu, does not reveal the presence of unusual compounds. The recoveries for 4 of the 43 compounds in the LCS Standard were high.

Data File : C:\HPCHEM\1\DATA\APR0405\6992.D
 Acq On : 6 Apr 2002 2:37 pm
 Sample : gc/ms scan 3/26
 Misc :
 MS Integration Params: GOOFY.P
 Quant Time: Apr 15 14:32 2002

Vial: 21
 Operator:
 Inst : GC/MS 209
 Multiplr: 2.00

Quant Results File: GCMS0408.RES

Quant Method : C:\HPCHEM\1\METHODS\GCMS0408.M (RTE Integrator)
 Title : 209 625/TCLP calibration table
 Last Update : Mon Apr 15 14:10:52 2002
 Response via : Initial Calibration
 DataAcq Meth : GCMS0403

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	12.25	152	469331	20.00	ug/l	-0.01
10) Naphthalene-d8	15.88	136	1715797	20.00	ug/l	-0.02
17) Acenaphthene-d10	21.19	164	974416	20.00	ug/l	-0.01
30) Phenanthrene-d10	25.63	188	1345202	20.00	ug/l	-0.02
39) Chrysene-d12	33.69	240	650631	20.00	ug/l	-0.03
45) Perylene-d12	37.93	264	352284	20.00	ug/l	-0.02

System Monitoring Compounds

28) TCMX	23.33	209	30902	11.77	ug/mL	0.00
Spiked Amount	10.000		Recovery	=	117.70%	
38) 2,4-DDD	0.00	235	0	0.00	ug/mL	
Spiked Amount	5.000		Recovery	=	0.00%	

Target Compounds

					Qvalue
2) N-nitroso-dimethyl amine	0.00	74	0	N.D.	
3) bis(2-Chloroethyl)ether	0.00	93	0	N.D.	
4) 1,3-Dichlorobenzene	0.00	146	0	N.D.	
5) 1,4-Dichlorobenzene	0.00	146	0	N.D.	
6) 1,2-Dichlorobenzene	0.00	146	0	N.D.	
7) 2,2'-oxybis(1-Chloropropan	0.00	45	0	N.D.	
8) N-Nitroso-di-n-propylamine	0.00	70	0	N.D.	
9) Hexachloroethane	0.00	117	0	N.D.	
11) Nitrobenzene	0.00	77	0	N.D.	
12) Isophorone	0.00	82	0	N.D.	
13) bis(2-Chloroethoxy)methane	0.00	93	0	N.D.	
14) 1,2,4-Trichlorobenzene	0.00	180	0	N.D.	
15) Naphthalene	0.00	128	0	N.D.	
16) Hexachlorobutadiene	0.00	225	0	N.D.	
18) Hexachlorocyclopentadiene	0.00	237	0	N.D.	
19) 2-Chloronaphthalene	0.00	162	0	N.D.	
20) Dimethylphthalate	0.00	163	0	N.D.	
21) 2,6-Dinitrotoluene	0.00	165	0	N.D.	d
22) Acenaphthylene	0.00	152	0	N.D.	
23) Acenaphthene	0.00	153	0	N.D.	
24) 2,4-Dinitrotoluene	0.00	165	0	N.D.	
25) Diethylphthalate	22.67	149	521	N.D.	
26) 4-Chlorophenyl-phenylether	0.00	204	0	N.D.	
27) Fluorene	0.00	166	0	N.D.	
29) Azobenzen/ 1,2-Diphenylhyd	0.00	77	0	N.D.	
31) N-Nitrosodiphenylamine	0.00	168	0	N.D.	
32) 4-Bromophenyl-phenylether	0.00	248	0	N.D.	

(#) = qualifier out of range (m) = manual integration

6992.D GCMS0408.M Mon Apr 15 14:32:59 2002

Page 1

Data File : C:\HPCHEM\1\DATA\APR0405\6992.D

Vial: 21

Acq On : 6 Apr 2002 2:37 pm

Operator:

Sample : gc/ms scan 3/26

Inst : GC/MS 209

Misc :

Multiplr: 2.00

MS Integration Params: GOOFY.P

Quant Time: Apr 15 14:32 2002

Quant Results File: GCMS0408.RES

Quant Method : C:\HPCHEM\1\METHODS\GCMS0408.M (RTE Integrator)

Title : 209 625/TCLP calibration table

Last Update : Mon Apr 15 14:10:52 2002

Response via : Initial Calibration

DataAcq Meth : GCMS0403

Compound	R.T.	QIon	Response	Conc Unit	Qvalue
33) Hexachlorobenzene	0.00	284	0	N.D.	
34) Phenanthrene	25.63	178	392	N.D.	
35) Anthracene	25.63	178	392	N.D.	
36) Di-n-butylphthalate	27.60	149	3756	N.D.	
37) Fluoranthene	0.00	202	0	N.D.	
40) Pyrene	0.00	202	0	N.D.	
41) Butylbenzylphthalate	0.00	149	0	N.D.	
42) Benzo(a)anthracene	33.69	228	1480	N.D.	
43) Bis(2-ethylhexyl)phthalate	0.00	149	0	N.D.	d
44) Chrysene	33.69	228	1480	N.D.	
46) Di-n-Octylphthalate	0.00	149	0	N.D.	
47) Benzo(b)fluoranthene	0.00	252	0	N.D.	
48) Benzo(k)fluoranthene	0.00	252	0	N.D.	
49) Benzo(a)pyrene	37.93	252	1292	N.D.	
50) Indeno(1,2,3-cd)pyrene	0.00	276	0	N.D.	
51) Dibenz(a,h)anthracene	0.00	278	0	N.D.	
52) Benzo(g,h,i)perylene	0.00	276	0	N.D.	

(#) = qualifier out of range (m) = manual integration

6992.D GCMS0408.M Mon Apr 15 14:33:00 2002

Page 2

Quantitation Report

Data File : C:\HPCHEM\1\DATA\APR0405\6992.D

Vial: 21

Acq On : 6 Apr 2002 2:37 pm

Operator:

Sample : gc/ms scan 3/26

Inst : GC/MS 209

Misc :

Multiplr: 2.00

MS Integration Params: GOOFY.P

Quant Time: Apr 15 14:32 2002


Quant Results File: GCMS0408.RES

Method : C:\HPCHEM\1\METHODS\GCMS0408.M (RTE Integrator)

Title : 209 625/TCLP calibration table

Last Update : Mon Apr 15 14:10:52 2002

Response via : Initial Calibration

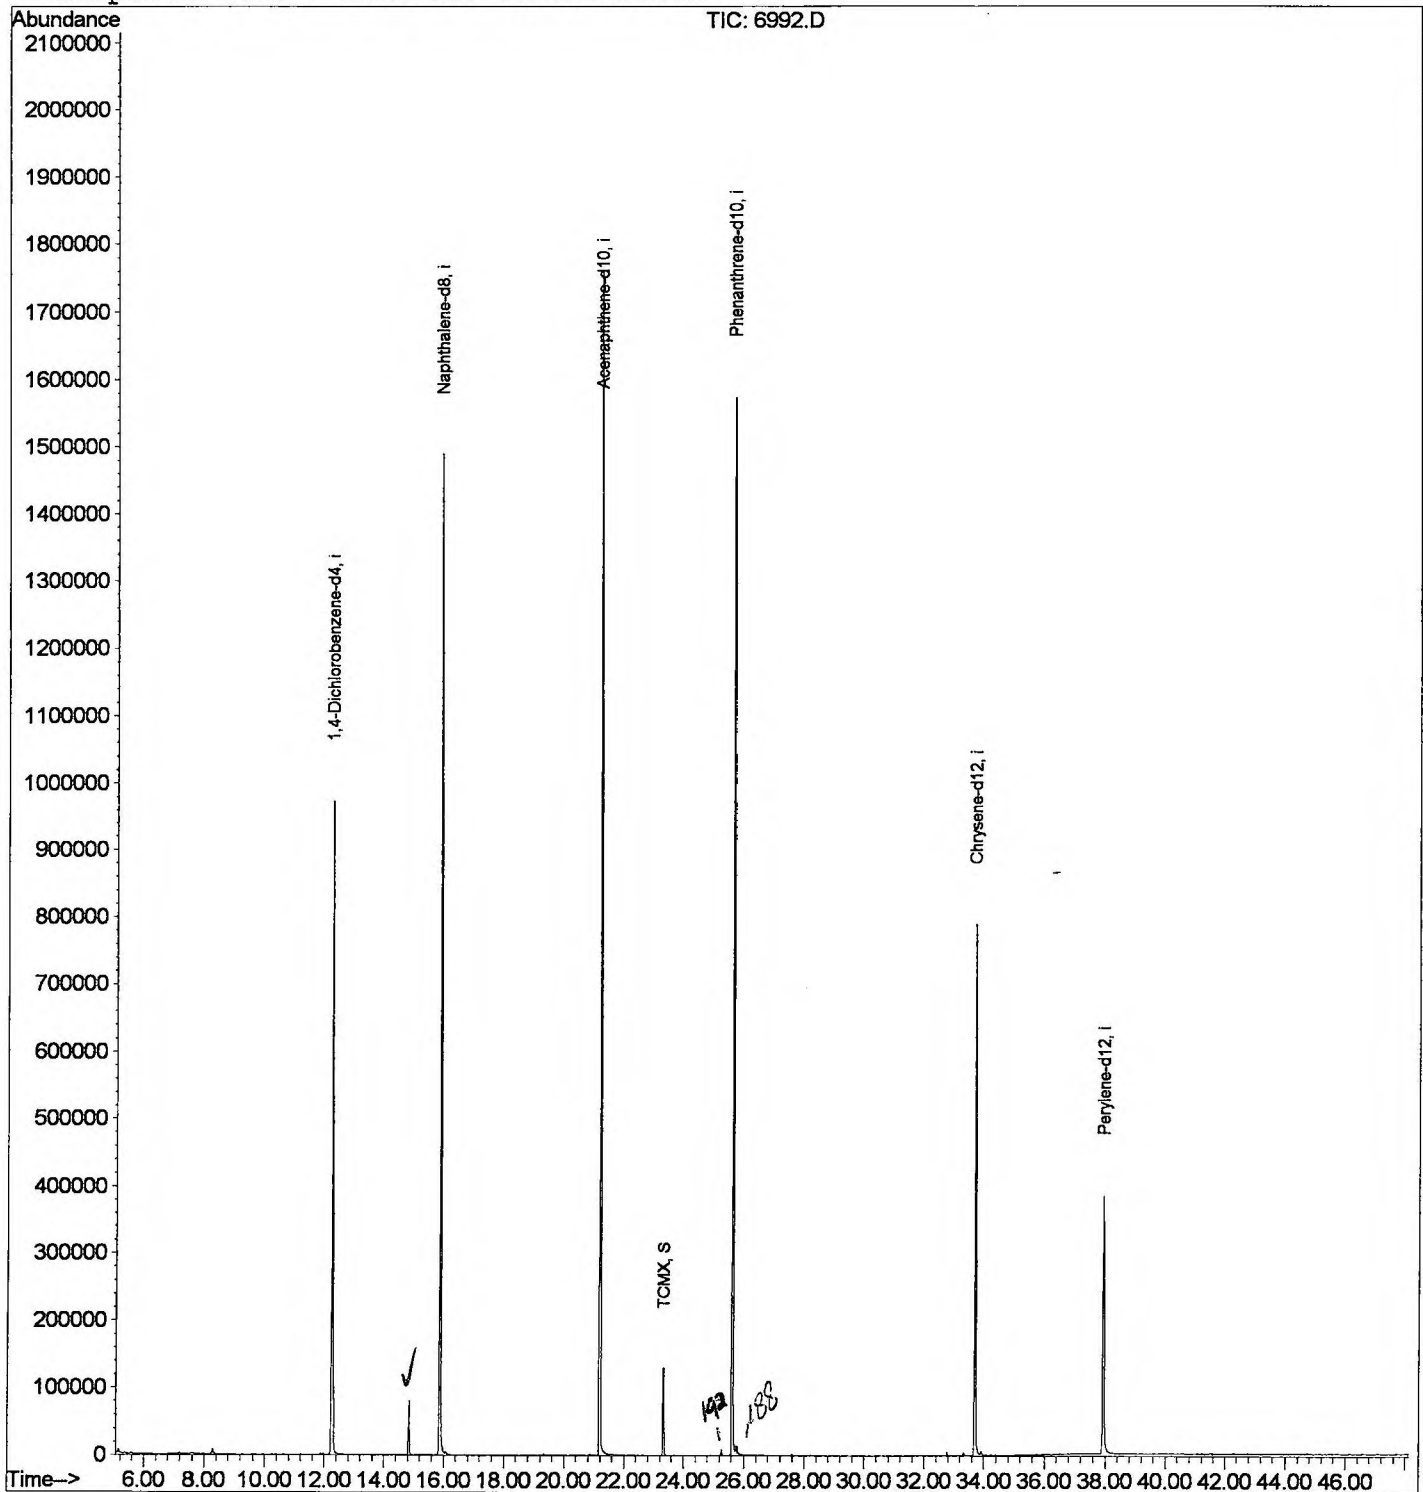

6992.D GCMS0408.M

Mon Apr 15 14:33:02 2002

Page 3

LSC Area Percent Report

Data File : C:\HPCHEM\1\DATA\APR0405\6992.D

Vial: 21

Acq On : 6 Apr 2002 2:37 pm

Operator:

Sample : gc/ms scan 3/26

Inst : GC/MS 209

Misc :

Multiplr: 2.00

MS Integration Params: LSCINT.P

Method : C:\HPCHEM\1\METHODS\GCMS0408.M (RTE Integrator)

Title : 209 625/TCLP calibration table

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	peak area	peak % max.	% of total
1	12.240	779	784	802	rVB	971819	2520434	68.27%	15.421%
2	14.847	1063	1068	1076	rVB	80576	157843	4.28%	0.966%
3	15.885	1174	1181	1195	rBV	1489127	3235352	87.64%	19.795%
4	21.191	1752	1759	1772	rBV	1761850	3691786	100.00%	22.587%
5	23.330	1984	1992	2000	rBV	129492	270733	7.33%	1.656%
6	25.634	2236	2243	2253	rBV	1573291	3395256	91.97%	20.773%
7	33.685	3114	3120	3140	rBV2	789528	1879062	50.90%	11.497%
8	37.927	3575	3582	3599	rBV2	383686	1194138	32.35%	7.306%




Sum of corrected areas: 16344604

6992.D GCMS0408.M

Mon Apr 15 14:43:50 2002

LSC Report - Integrated Chromatogram

File : C:\HPCHEM\1\DATA\APR0405\6992.D
 Operator :
 Acquired : 6 Apr 2002 2:37 pm using AcqMethod GCMS0403
 Instrument : GC/MS 209
 Sample Name: gc/ms scan 3/26
 Misc Info :
 Vial Number: 21
 Quant File :GCMS0408.RES (RTE Integrator)

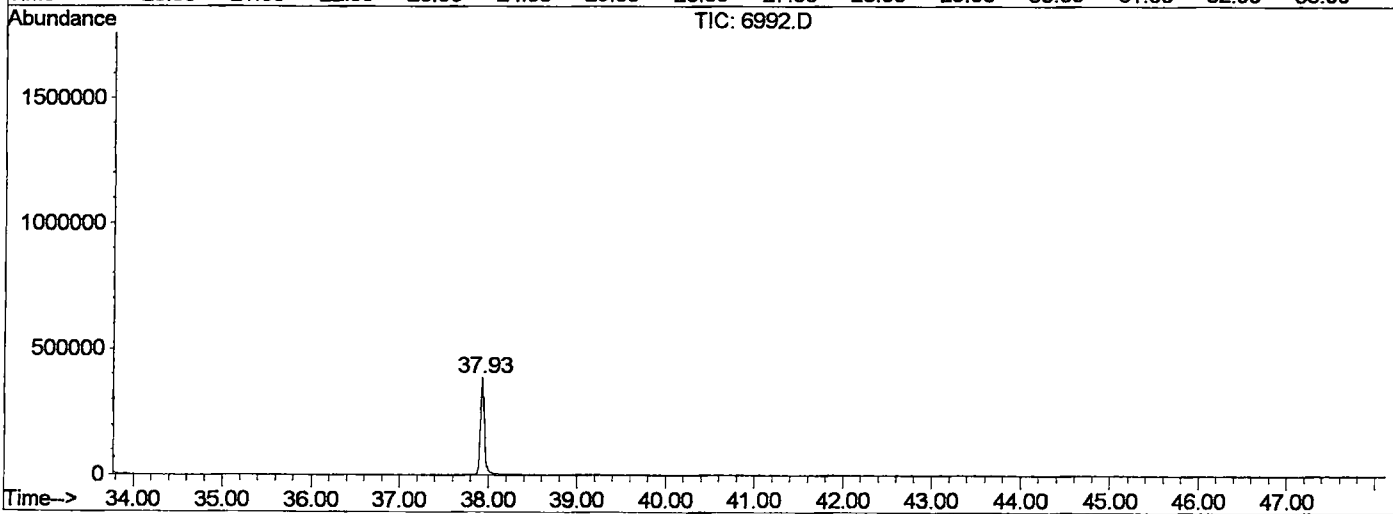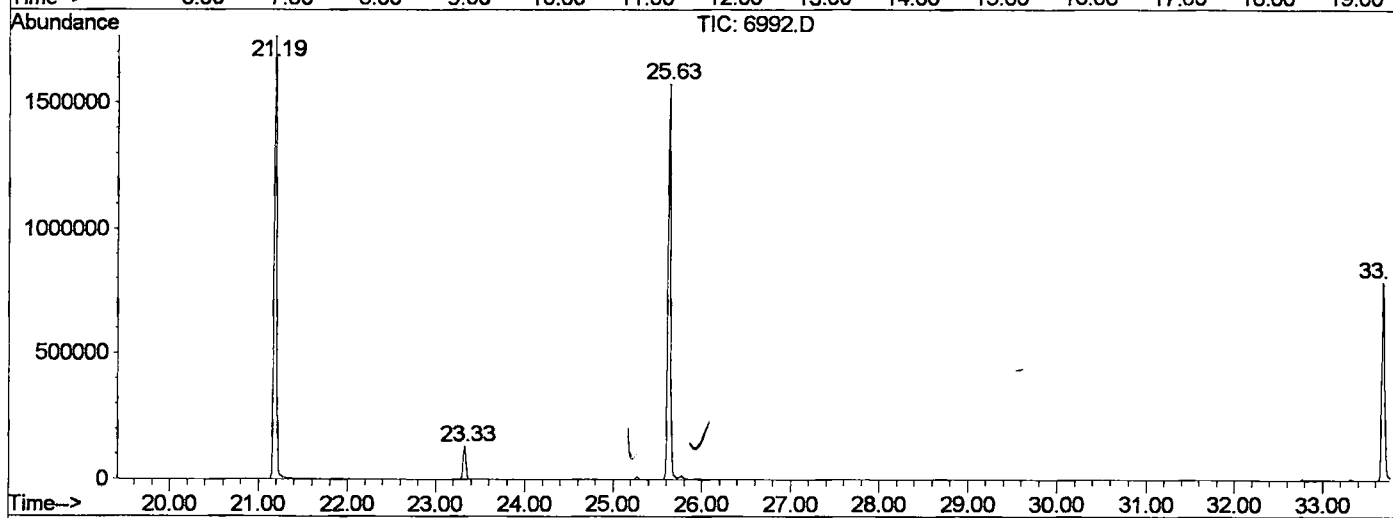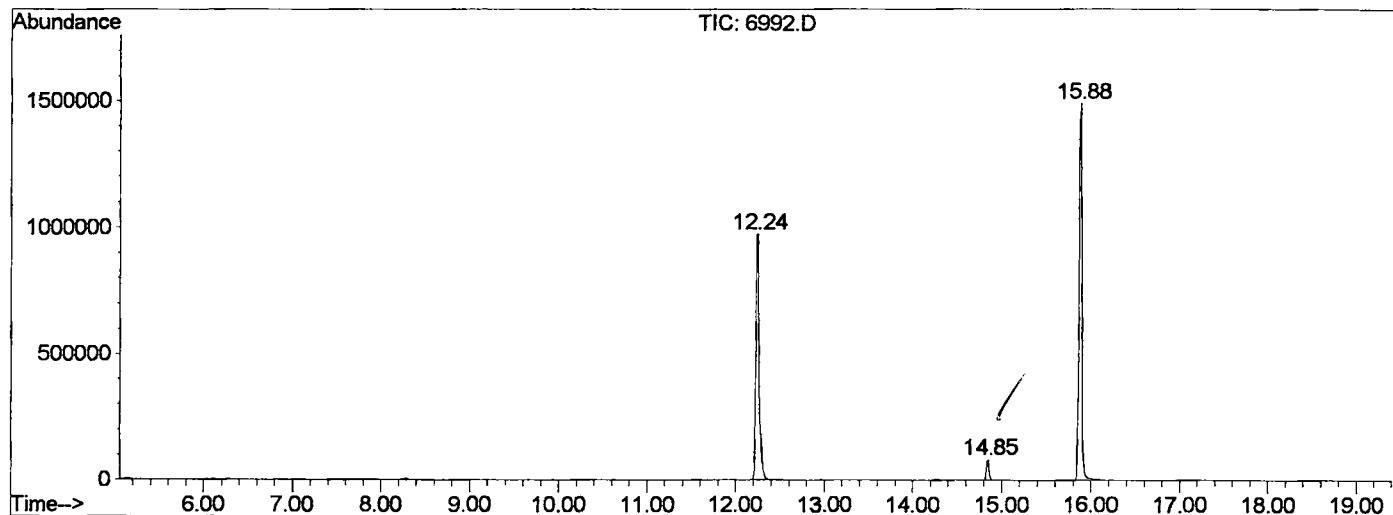

6992.D GCMS0408.M Mon Apr 15 14:43:51 2002

Library Search Compound Report

Data File : C:\HPCHEM\1\DATA\APR0405\6992.D

Acq On : 6 Apr 2002 2:37 pm

Sample : gc/ms scan 3/26

Misc :

MS Integration Params: LSCINT.P

Vial: 21

Operator:

Inst : GC/MS 209

Multiplr: 2.00

Quant Method : C:\HPCHEM\1\METHODS\GCMS0408.M (RTE Integrator)


Title : 209 625/TCLP calibration table

Library : C:\DATABASE\NBS75K.L

Peak Number 1 Cyclopentasiloxane, decamethyl Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
14.85	1.95 ug/l	157843	Naphthalene-d8	15.88

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	Cyclopentasiloxane, decamethyl-	370	C10H30O5Si5	000541-02-6	76
2		3,4-Dihydroxybenzyl alcohol, tris(tr	356	C16H32O3Si3	068595-79-9	58
3		3,4-Dihydroxymandelic acid, ethyl e	428	C19H36O5Si3	000000-00-0	47
4		Phenethylamine, N-methyl-.beta.,3,4	399	C18H37NO3Si3	010538-85-9	43

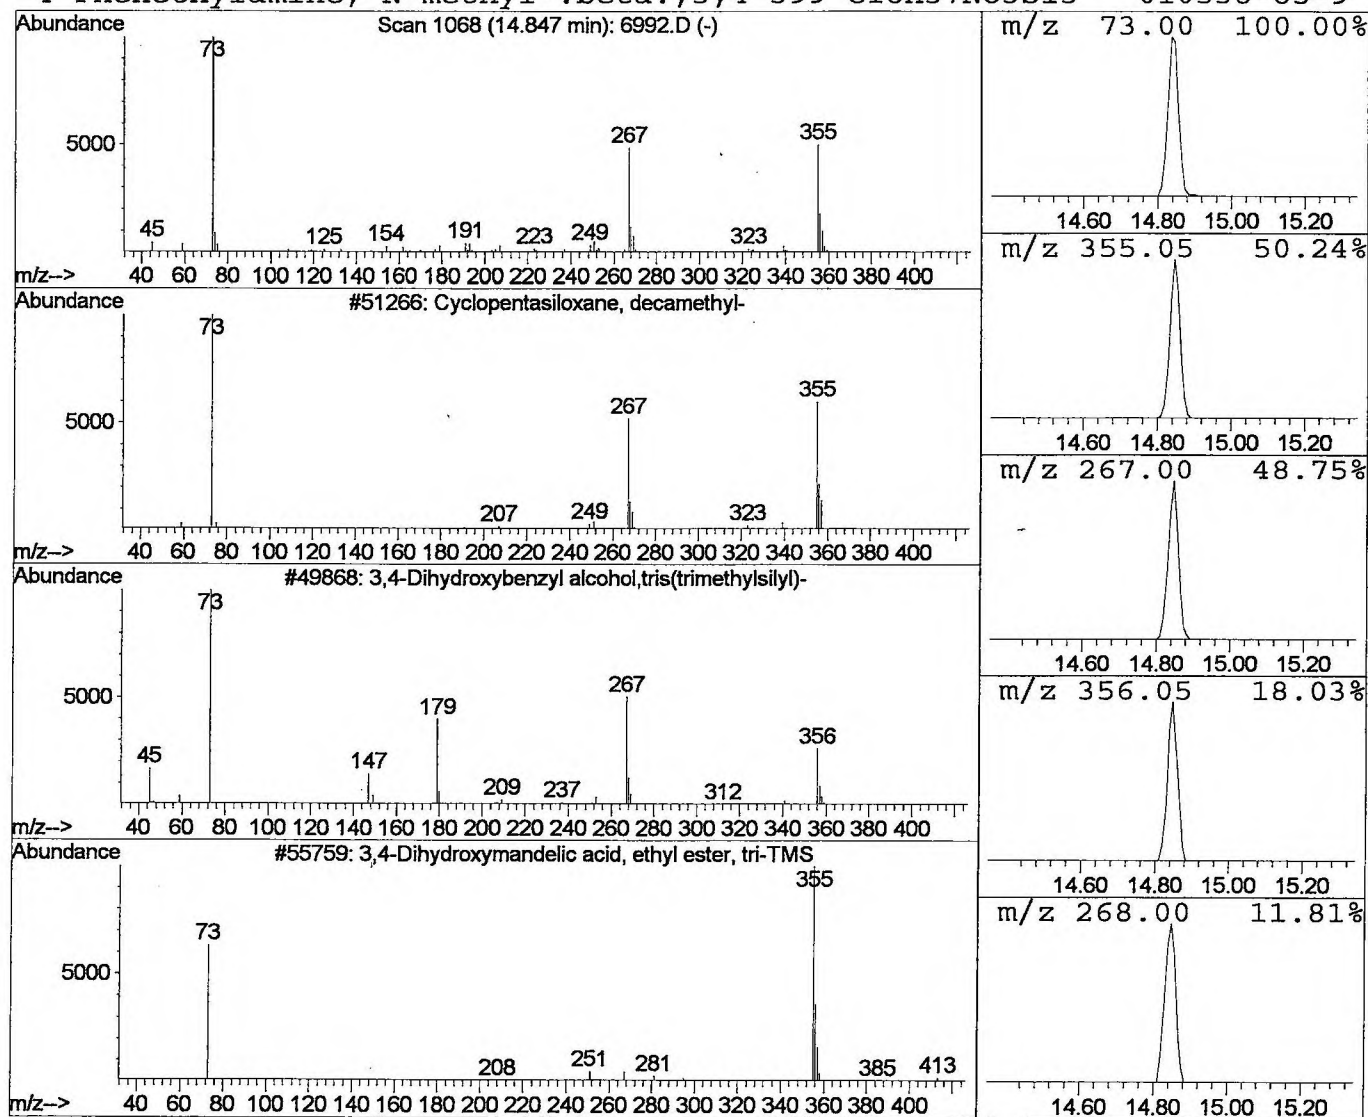

Tentatively Identified Compound (LSC) summary

Operator ID: Date Acquired: 6 Apr 2002 2:37 pm
 Data File: C:\HPCHEM\1\DATA\APR0405\6992.D
 Name: gc/ms scan 3/26
 Misc:
 Method: C:\HPCHEM\1\METHODS\GCMS0408.M (RTE Integrator)
 Title: 209 625/TCLP calibration table
 Library Searched: C:\DATABASE\NBS75K.L

TIC Top Hit name	RT	EstConc	Units	Area	IntStd	ISRT	ISArea	ISConc
Cyclopentasiloxane,	14.85	2.0	ug/l	157843	ISTD02	15.88	3235350	20.0

6992.D GCMS0408.M Mon Apr 15 14:43:52 2002