

User: Vinci, David L
Westchester Dept. of Labs & Research
Date: 05/06/2002 Time: 10:29:06

Sample: AE08481
Analysis: \$GCMS GCMS Scan For Unknowns
Units: ug
Started: 5/6/02 10:28 Ended: 5/6/02 10:28 Analyst: DLV
Page: 1

	Component Name	Viol	Result	Qualifier	MDL
1	Other unknown compounds		.		
2	Surr_2,4-DDD		94		10.0

Comments for Sample AE08481 - Analysis \$GCMS

Westchester Dept. of Labs & Research

User: Vinci, David L

Date: 05-06-2002 Time: 10:29:33

The GCMS scan, from 35 to 550 amu, does not reveal the presence of unusual compounds.

Quantitation Report

(QT Reviewed)

Data File : C:\HPCHEM\1\DATA\MAY0202\8481.D
 Acq On : 3 May 2002 4:38 am
 Sample : GC/MS SCAN 4/22
 Misc :
 MS Integration Params: GOOFY.P
 Quant Time: May 3 9:55 2002

Vial: 15
 Operator:
 Inst : 209
 Multiplr: 1.00

Quant Results File: GCMS0501.RES

Quant Method : C:\HPCHEM\1\METHODS\GCMS0501.M (RTE Integrator)
 Title : 209 625/TCLP calibration table
 Last Update : Wed May 01 10:40:31 2002
 Response via : Initial Calibration
 DataAcq Meth : GCMS0501

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	12.19	152	371861	40.00	ug/l	-0.02
10) Naphthalene-d8	15.83	136	1375800	40.00	ug/l	-0.02
17) Acenaphthene-d10	21.14	164	742158	40.00	ug/l	-0.01
30) Phenanthrene-d10	25.58	188	1019194	40.00	ug/l	-0.01
38) Chrysene-d12	33.64	240	633424	40.00	ug/l	-0.03
44) Perylene-d12	37.87	264	444964	40.00	ug/l	-0.01

System Monitoring Compounds

28) TCMX	23.27	209	34012	9.41	ug/L	-0.02
Spiked Amount	10.000		Recovery	=	94.10%	

Target Compounds

					Qvalue
2) N-nitroso-dimethyl amine	0.00	74	0	N.D.	
3) bis(2-Chloroethyl)ether	0.00	93	0	N.D.	
4) 1,3-Dichlorobenzene	0.00	146	0	N.D.	
5) 1,4-Dichlorobenzene	0.00	146	0	N.D.	
6) 1,2-Dichlorobenzene	0.00	146	0	N.D.	
7) 2,2'-oxybis(1-Chloropropan	0.00	45	0	N.D.	
8) N-Nitroso-di-n-propylamine	0.00	70	0	N.D.	
9) Hexachloroethane	0.00	117	0	N.D.	
11) Nitrobenzene	13.42	77	766	N.D.	
12) Isophorone	0.00	82	0	N.D.	
13) bis(2-Chloroethoxy)methane	0.00	93	0	N.D.	
14) 1,2,4-Trichlorobenzene	0.00	180	0	N.D.	
15) Naphthalene	0.00	128	0	N.D.	
16) Hexachlorobutadiene	0.00	225	0	N.D.	
18) Hexachlorocyclopentadiene	0.00	237	0	N.D.	
19) 2-Chloronaphthalene	0.00	162	0	N.D.	
20) Dimethylphthalate	0.00	163	0	N.D.	
21) 2,6-Dinitrotoluene	0.00	165	0	N.D.	d
22) Acenaphthylene	0.00	152	0	N.D.	
23) Acenaphthene	0.00	153	0	N.D.	
24) 2,4-Dinitrotoluene	0.00	165	0	N.D.	
25) Diethylphthalate	22.62	149	864	N.D.	
26) 4-Chlorophenyl-phenylether	0.00	204	0	N.D.	
27) Fluorene	0.00	166	0	N.D.	
29) Azobenzen/ 1,2-Diphenylhyd	0.00	77	0	N.D.	
31) N-Nitrosodiphenylamine	0.00	168	0	N.D.	
32) 4-Bromophenyl-phenylether	0.00	248	0	N.D.	
33) Hexachlorobenzene	0.00	284	0	N.D.	
34) Phenanthrene	25.58	178	207	N.D.	

(#) = qualifier out of range (m) = manual integration

8481.D GCMS0501.M Fri May 03 09:56:15 2002

Page 1

Quantitation Report (QT Reviewed)

Data File : C:\HPCHEM\1\DATA\MAY0202\8481.D
 Acq On : 3 May 2002 4:38 am
 Sample : GC/MS SCAN 4/22
 Misc :
 MS Integration Params: GOOFY.P
 Quant Time: May 3 9:55 2002

Vial: 15
 Operator:
 Inst : 209
 Multiplr: 1.00

Quant Results File: GCMS0501.RES

Quant Method : C:\HPCHEM\1\METHODS\GCMS0501.M (RTE Integrator)
 Title : 209 625/TCLP calibration table
 Last Update : Wed May 01 10:40:31 2002
 Response via : Initial Calibration
 DataAcq Meth : GCMS0501

Compound	R.T.	QIon	Response	Conc	Unit	Qvalue
35) Anthracene	25.58	178	207	N.D.		
36) Di-n-butylphthalate	27.55	149	3622	N.D.		
37) Fluoranthene	0.00	202	0	N.D.		
39) Pyrene	0.00	202	0	N.D.		
40) Butylbenzylphthalate	0.00	149	0	N.D.		
41) Benzo(a)anthracene	33.64	228	1526	N.D.		
42) Bis(2-ethylhexyl)phthalate	33.87	149	2188	N.D.		
43) Chrysene	33.72	228	200	N.D.		
45) Di-n-Octylphthalate	0.00	149	0	N.D.		
46) Benzo(b)fluoranthene	36.77	252	563	N.D.		
47) Benzo(k)fluoranthene	36.77	252	293	N.D.		
48) Benzo(a)pyrene	37.86	252	1644	N.D.		
49) Indeno(1,2,3-cd)pyrene	0.00	276	0	N.D.		
50) Dibenz(a,h)anthracene	0.00	278	0	N.D.		
51) Benzo(g,h,i)perylene	0.00	276	0	N.D.		

(#) = qualifier out of range (m) = manual integration
 8481.D GCMS0501.M Fri May 03 09:56:16 2002


Quantitation Report

Data File : C:\HPCHEM\1\DATA\MAY0202\8481.D
Acq On : 3 May 2002 4:38 am
Sample : GC/MS SCAN 4/22
Misc :
MS Integration Params: GOOFY.P
Quant Time: May 3 9:55 2002

Vial: 15
Operator:
Inst : 209
Multiplr: 1.00

Quant Results File: GCMS0501.RES

Method : C:\HPCHEM\1\METHODS\GCMS0501.M (RTE Integrator)
Title : 209 625/TCLP calibration table
Last Update : Wed May 01 10:40:31 2002
Response via : Initial Calibration

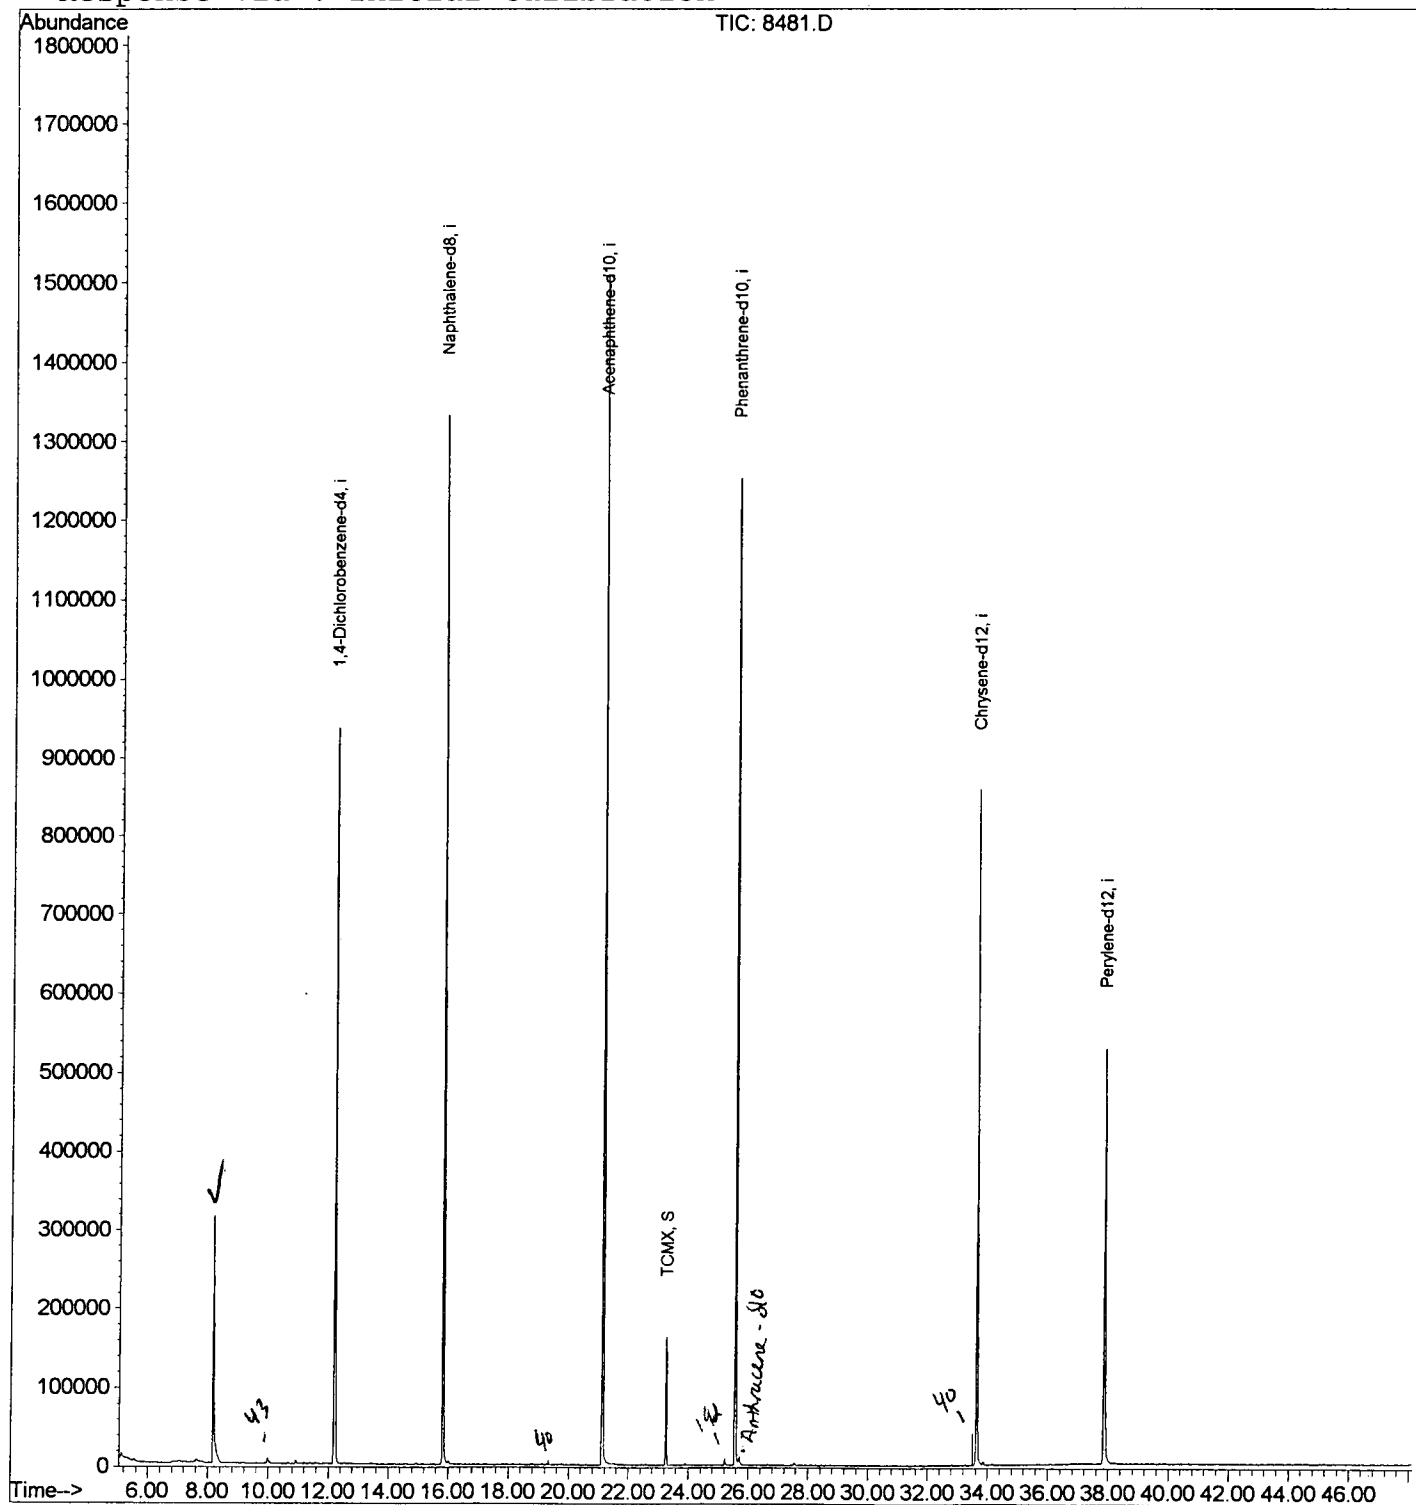

LSC Area Percent Report

Data File : C:\HPCHEM\1\DATA\MAY0202\8481.D
 Acq On : 3 May 2002 4:38 am
 Sample : GC/MS SCAN 4/22
 Misc :
 MS Integration Params: LSCINT.P

Vial: 15
 Operator:
 Inst : 209
 Multiplr: 1.00

Method : C:\HPCHEM\1\METHODS\GCMS0501.M (RTE Integrator)
 Title : 209 625/TCLP calibration table
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Signal : TIC




peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	peak area	peak % max.	% of total
1	8.162	338	341	368	rBV	311979	762287	25.04%	4.995%
2	12.194	776	781	801	rVB	933996	2162518	71.04%	14.171%
3	15.832	1172	1178	1195	rBV	1329584	2755720	90.53%	18.059%
4	21.138	1751	1757	1772	rBV	1506790	3044098	100.00%	19.948%
5	23.273	1983	1990	1996	rBV	161841	322182	10.58%	2.111%
6	25.582	2235	2242	2253	rBV2	1250694	2751675	90.39%	18.032%
7	33.637	3114	3121	3139	rBV2	857712	1920517	63.09%	12.585%
8	37.871	3575	3583	3605	rBV	524839	1540845	50.62%	10.097%

Sum of corrected areas: 15259842

8481.D GCMS0501.M Fri May 03 12:23:17 2002

LSC Report - Integrated Chromatogram

File : C:\HPCHEM\1\DATA\MAY0202\8481.D
 Operator :
 Acquired : 3 May 2002 4:38 am using AcqMethod GCMS0501
 Instrument : 209
 Sample Name: GC/MS SCAN 4/22
 Misc Info :
 Vial Number: 15
 Quant File :GCMS0501.RES (RTE Integrator)

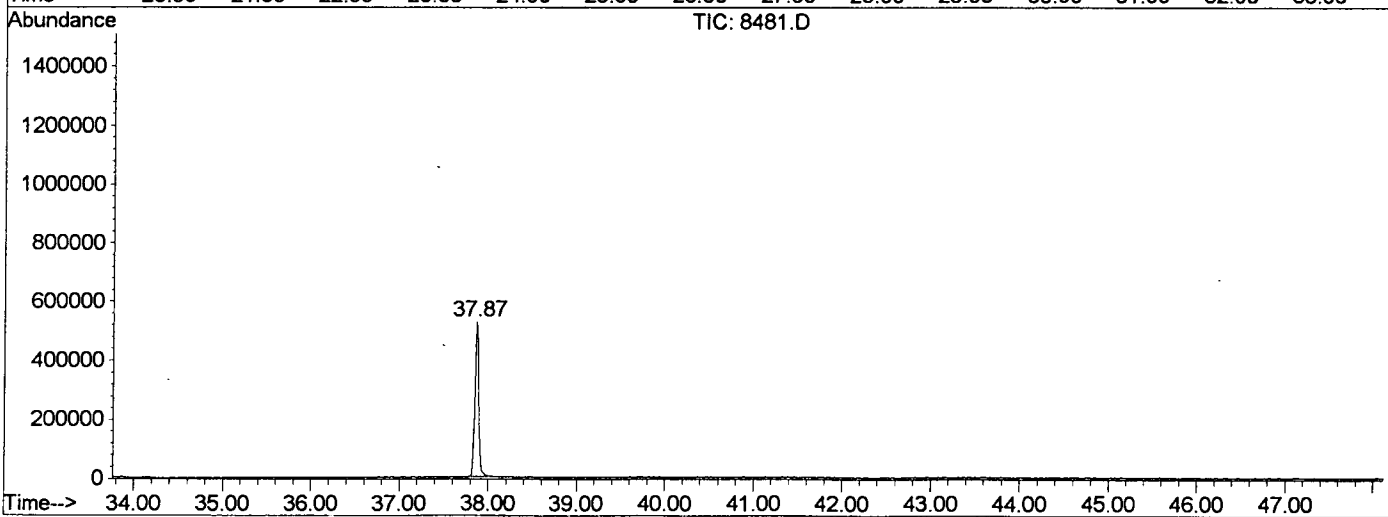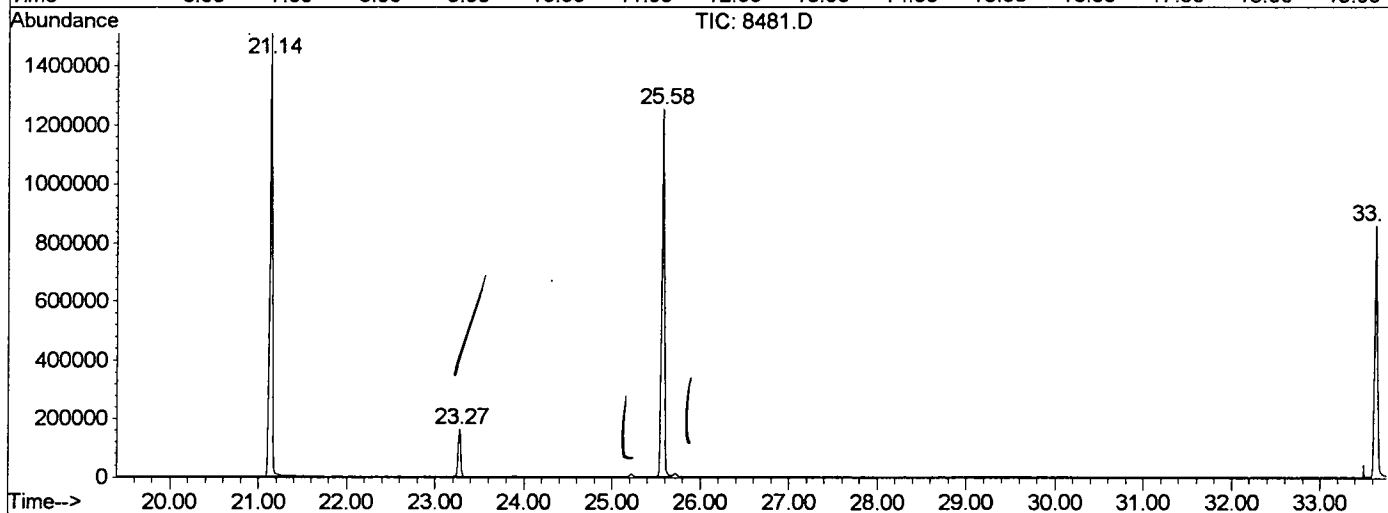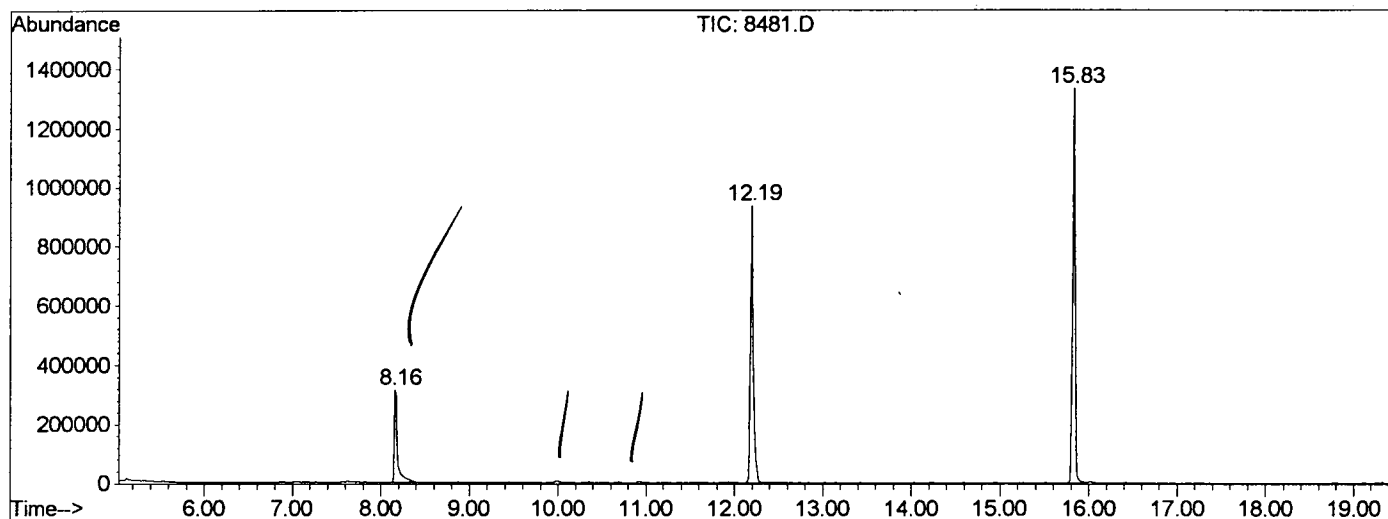

8481.D GCMS0501.M Fri May 03 12:23:18 2002

Library Search Compound Report

Data File : C:\HPCHEM\1\DATA\MAY0202\8481.D
Acq On : 3 May 2002 4:38 am
Sample : GC/MS SCAN 4/22
Misc :
MS Integration Params: LSCINT.P


Vial: 15
Operator:
Inst : 209
Multiplr: 1.00

Quant Method : C:\HPCHEM\1\METHODS\GCMS0501.M (RTE Integrator)
Title : 209 625/TCLP calibration table
Library : C:\DATABASE\NBS75K.L

Peak Number 1 2-Pentanone, 4-hydroxy-4-methy Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
8.16	14.10 ug/l	762287	1,4-Dichlorobenzene-d4	12.19

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	78		
2	3-Hydroxy-2-pentanone	102	C5H10O2	003142-66-3	9		
3	CH2=CHCH2C(O)OCH3	100	C5H8O2	003724-55-8	8		
4	Propanenitrile, 3-ethoxy-	99	C5H9NO	002141-62-0	7		

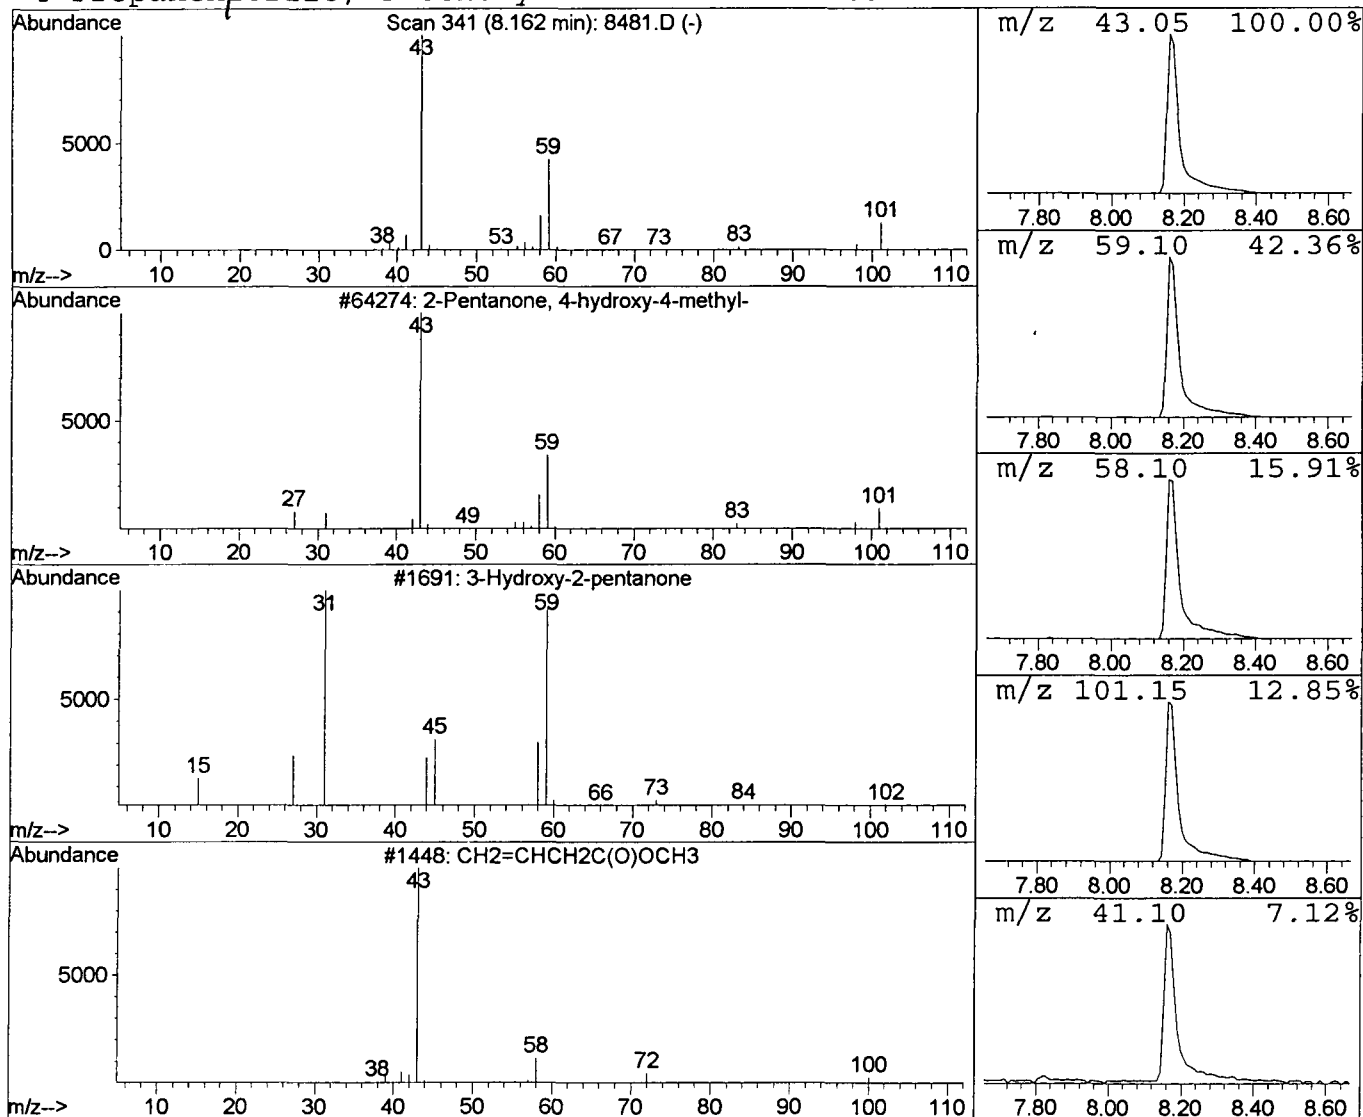

Tentatively Identified Compound (LSC) summary

Operator ID: Date Acquired: 3 May 2002 4:38 am
 Data File: C:\HPCHEM\1\DATA\MAY0202\8481.D
 Name: GC/MS SCAN 4/22
 Misc:
 Method: C:\HPCHEM\1\METHODS\GCMS0501.M (RTE Integrator)
 Title: 209 625/TCLP calibration table
 Library Searched: C:\DATABASE\NBS75K.L

TIC Top Hit name	RT	EstConc	Units	Area	IntStd	ISRT	ISArea	ISConc
2-Pentanone, 4-hydro	8.16	14.1	ug/l	762287	ISTD01	12.19	2162520	40.0
8481.D GCMS0501.M	Fri May 03 12:23:19 2002							