

Comment: INST 209; SUMX0.25SUMX0.50

Operator: 209 GALOS

Data Path: C:\HPCHEM\1\data\feb1502\

Pre-Seq Cmd:

Post-Seq Cmd:

Method Sections To Run	On A Barcode Mismatch
(X) Full Method	(X) Inject Anyway
() Reprocessing Only	() Don't Inject

Line	Type	Vial	DataFile	Method	Sample Name
1	Sample	1	DFTPP	GCMS0208	
2	Sample	2	CAL10	GCMS0208	
3	Sample	3	LB	GCMS0208	gc/ms scan 1/16
4	Sample	4	REF	GCMS0208	gc/ms scan 1/16
5	Sample	5	1143	GCMS0208	gc/ms scan 1/16
6	Sample	6	1156	GCMS0208	gc/ms scan 1/16
7	Sample	7	1153	GCMS0208	gc/ms scan 1/16
8	Sample	8	1155	GCMS0208	gc/ms scan 1/16
9	Sample	9	1154	GCMS0208	gc/ms scan 1/16
10	Sample	10	1137	GCMS0208	gc/ms scan 1/16
11	Sample	11	LBA	GCMS0208	gc/ms scan 2/15
12	Sample	12	REFA	GCMS0208	gc/ms scan 2/15
13	Sample	13	REFA2	GCMS0208	gc/ms scan 2/15
14	Sample	14	1940	GCMS0208	re-extract
15	Sample	15	1941	GCMS0208	re-extract
16	Sample	16	1943	GCMS0208	re-extract
17	Sample	17	3438	GCMS0208	gc/ms scan 2/15
18	Sample	18	3439	GCMS0208	gc/ms scan 2/15
19	Sample	19	3440	GCMS0208	gc/ms scan 2/15
20	Sample	20	3441	GCMS0208	gc/ms scan 2/15
21	Sample	21	3454	GCMS0208	gc/ms scan 2/15
22	Sample	22	3471	GCMS0208	gc/ms scan 2/15
23	Sample	23	3472	GCMS0208	gc/ms scan 2/15
24	Sample	1	DFTPP1	GCMS0208	gc/ms scan 2/15
25	Sample	2	CAL10A	GCMS0208	gc/ms scan 2/15
26	Sample	24	LBB	GCMS0208	gc/ms scan 1/17
27	Sample	25	REFB	GCMS0208	gc/ms scan 1/17
28	Sample	26	1226	GCMS0208	gc/ms scan 1/17
29	Sample	27	1225	GCMS0208	gc/ms scan 1/17
30	Sample	28	1222	GCMS0208	gc/ms scan 1/17
31	Sample	29	1043	GCMS0208	gc/ms scan 1/17
32	Sample	30	1041	GCMS0208	gc/ms scan 1/17
33	Sample	31	LBC	GCMS0208	gc/ms scan 1/17
34	Sample	32	REFC	GCMS0208	gc/ms scan 1/17
35	Sample	33	1224	GCMS0208	gc/ms scan 1/17
36	Sample	34	1223	GCMS0208	gc/ms scan 1/17
37	Sample	35	1221	GCMS0208	gc/ms scan 1/17
38	Sample	36	1220	GCMS0208	gc/ms scan 1/17
39	Sample	37	1230	GCMS0208	gc/ms scan 1/17
40	Sample	38	1231	GCMS0208	gc/ms scan 1/17
41	Sample	39	1232	GCMS0208	gc/ms scan 1/17
42	Sample	40	1227	GCMS0208	gc/ms scan 1/17

Last Modified: Mon Feb 18 10:54:00 2002

Page: 1

DFTPP

Data File : C:\HPCHEM\1\DATA\FEB1502\DFTPP1.D

Acq On : 16 Feb 2002 1:45 pm

Sample : gc/ms scan 2/15

Misc :

MS Integration Params: GOOFY.P

Method : C:\HPCHEM\1\METHODS\GCMS0208.M (RTE Integrator)


Title : 209 625/TCLP calibration table

Vial: 1

Operator: 209 GALOS

Inst : GC/MS 209

Multiplr: 1.00

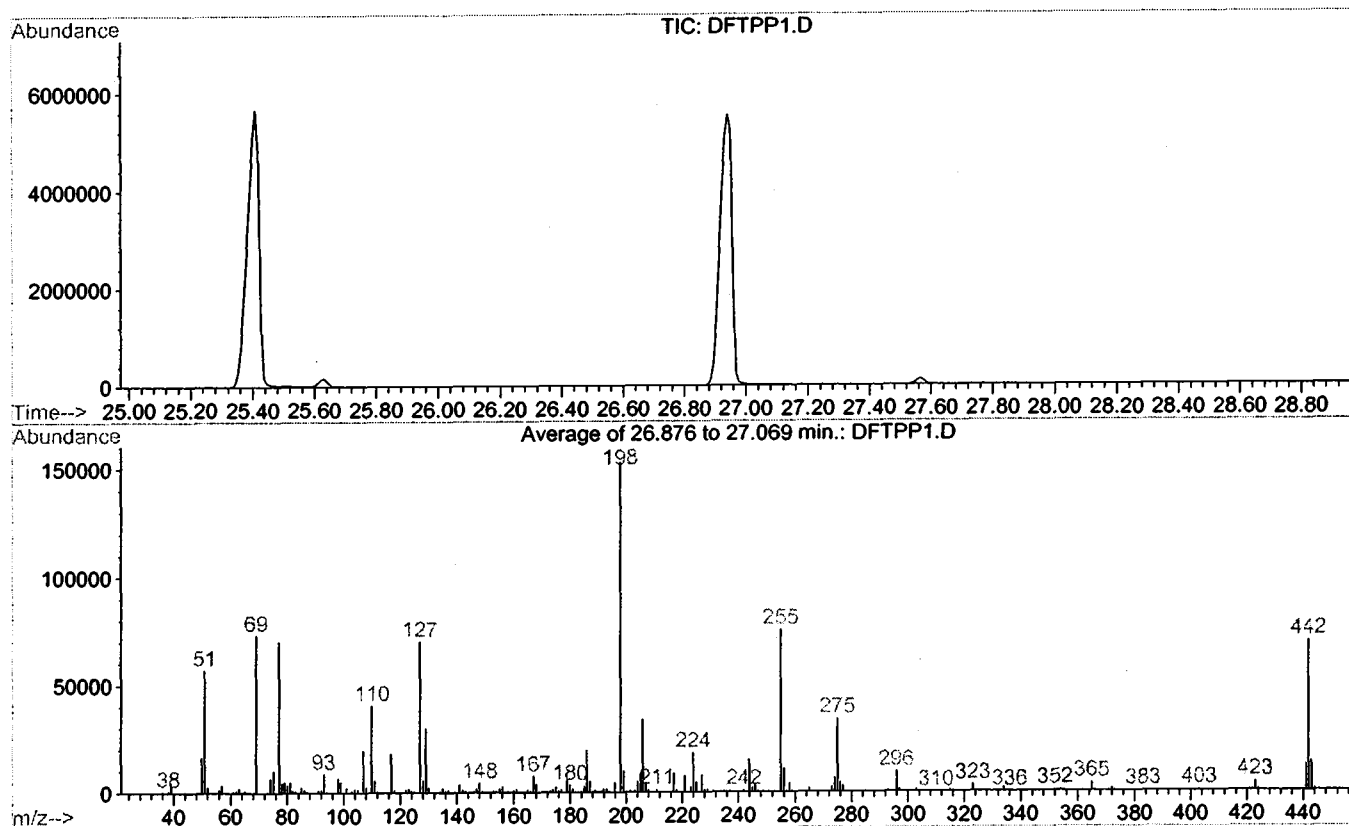

Spectrum Information: Average of 26.876 to 27.069 min.

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	30	60	37.4	57069	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	48.0	73387	PASS
70	69	0.00	2	0.1	67	PASS
127	198	40	60	46.1	70485	PASS
197	198	0.00	1	0.0	0	PASS
198	198	100	100	100.0	152787	PASS
199	198	5	9	6.6	10061	PASS
275	198	10	30	22.4	34208	PASS
365	198	1	100	2.6	4017	PASS
441	443	0.01	100	90.5	12294	PASS
442	198	40	110	45.7	69840	PASS
443	442	17	23	19.4	13579	PASS

DFTPP1.D GCMS0208.M

Wed Feb 20 13:53:48 2002